


WARNING

FAILURE TO FOLLOW THESE INSTRUCTIONS MAY RESULT IN SERIOUS INJURY.

1. When assembling and adjusting chair height upward or downward, gently push up on the toggle. Do not use excessive force to push down on the toggle.
2. Do not over-extend or use excessive force when adjusting the chair angle.
3. Do not touch the reclining mechanism to avoid possible falling or unexpected head injury when you are rocking the chair.
Be sure to put the rocking lever into the "Lock" position when fully reclining the chair.
4. When fully reclining the OsmoChair without leg rest, both feet should remain on the ground. Sudden or excessive force on the backrest could result in the chair tipping, as could horseplay, and both should be avoided.
5. The chair is for sitting and reclining only. Do not use as a stepstool, wheelchair or other purpose.
6. The chair is designed for only one person's use at a time. Please do not use as a stepstool or for kneeling.
7. The armrests are not designed for sitting upon. The edge of the seat is for supporting the knees. Do not sit on the edge of the chair.
8. All parts should be checked monthly to avoid unexpected injury due to loosen bolts or parts.
In the event parts are loose, missing or damaged, please contact Autonomous and do not use the product.
9. Keep out of reach of children under the age of 10 unless assistance from and adult is provided.
10. Avoid leaving the chair in direct sunlight to prevent fading or peeling off.
Clean with gentle cleaners when necessary. Do not scrub excessively.


EazeeChairs

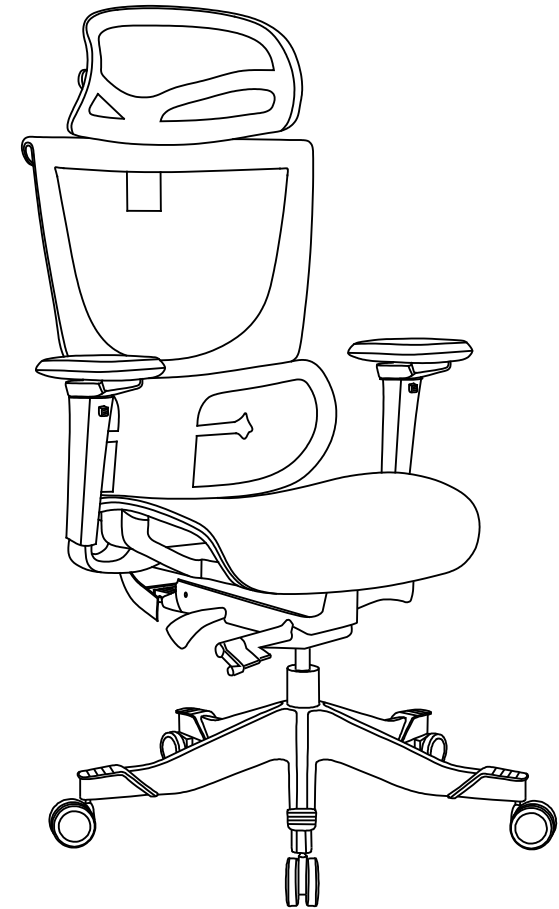

Customer Service: hi@eazeechairs.com
Website: www.eazeechairs.com

COMPONENTS

A



B




C




D



E



F



G



H



HARDWARE/TOOLS

I



(M8*20/M8/M8*16*2) x 3

J



(M6*30/M6/M6*15*1.5) x 10


K




Function 5




Handrails, 270 degrees.



Function 6

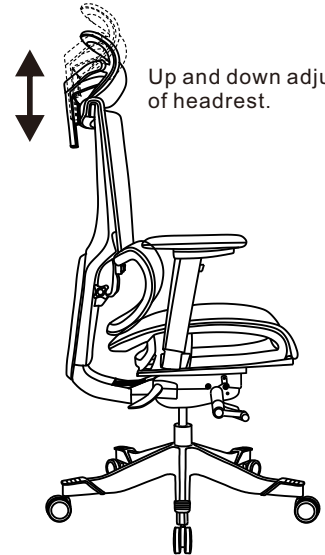


Up and down adjustment of headrest.

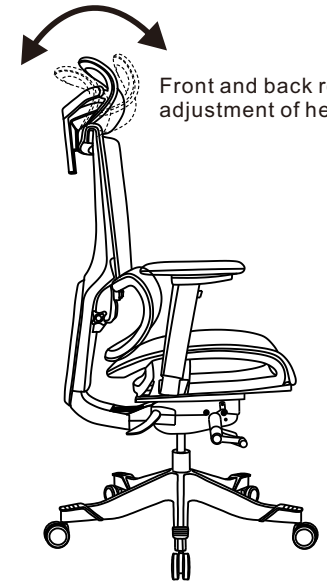

Front and back rotation adjustment of headrest.

Function 3

Handle raised downward, leaning back adjustment; handle raised upward, leaning back locking.

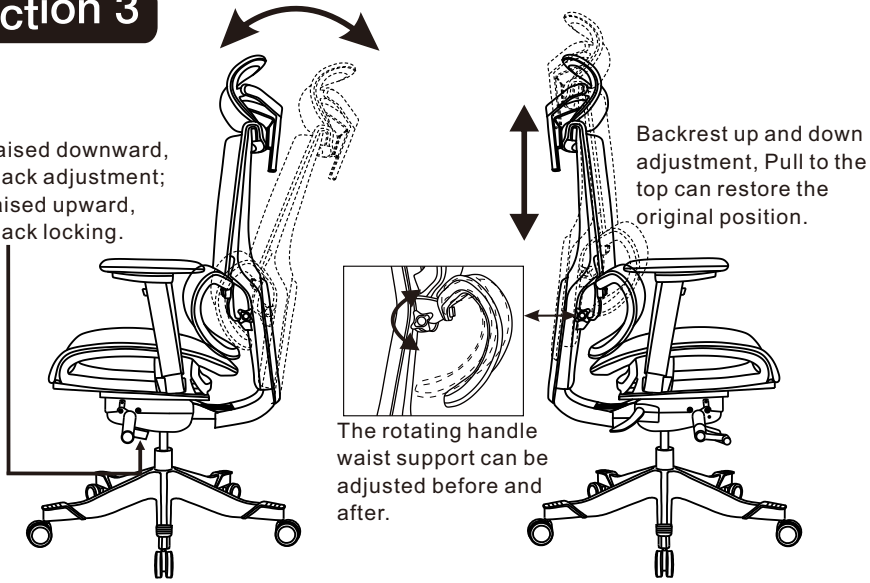


Backrest up and down adjustment, Pull to the top can restore the original position.


The rotating handle waist support can be adjusted before and after.

Step 1


Insert 5 Wheels to the holes on each prong of chair Base.

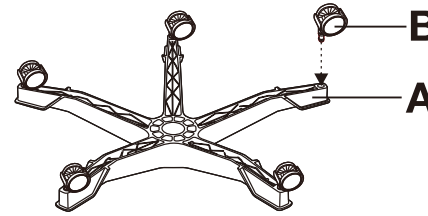


Step 2

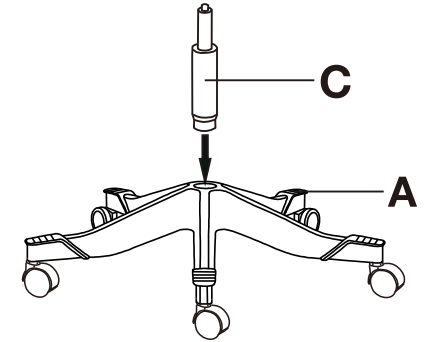

Function 4

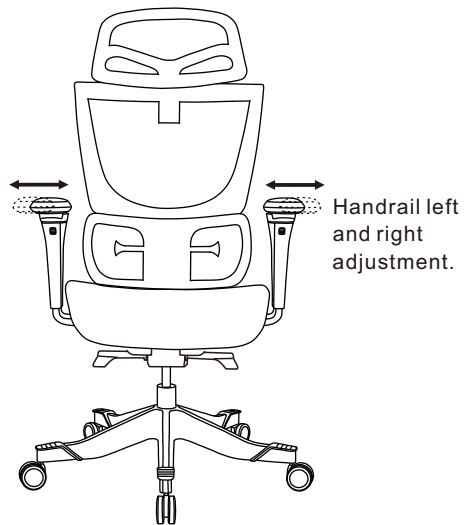


Handrail left and right adjustment.

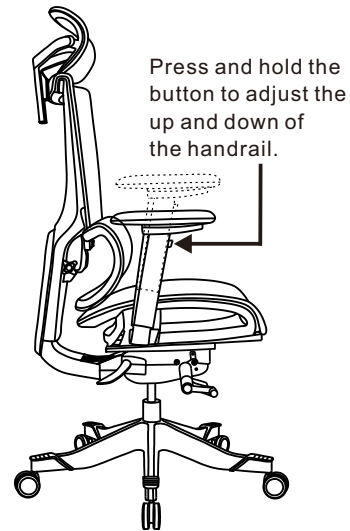


Press and hold the button to adjust the up and down of the handrail.


Step 3

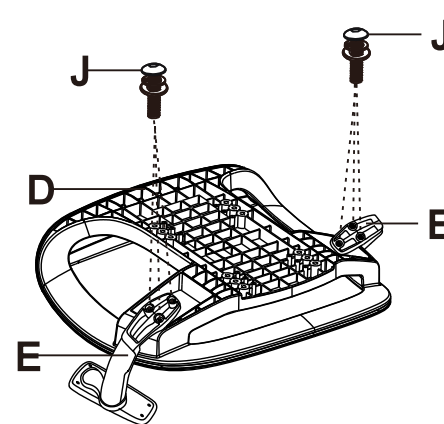


Step 4

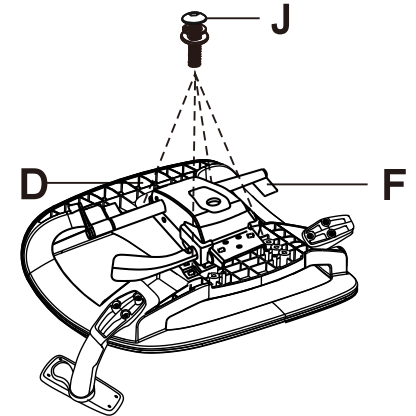


Step 5

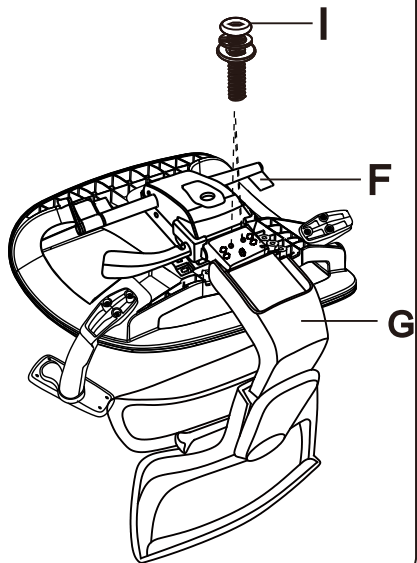


Step 6

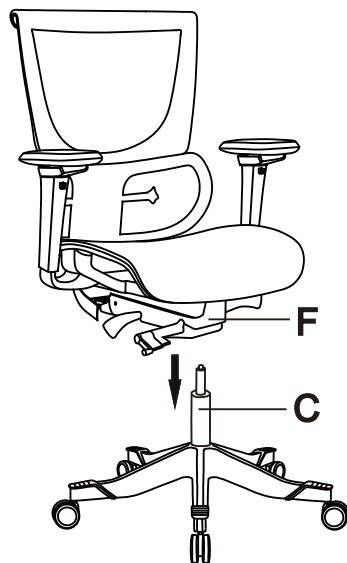

Function 1

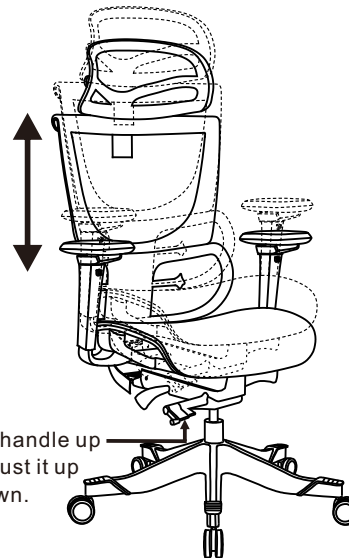


Lift the handle up and adjust it up and down.

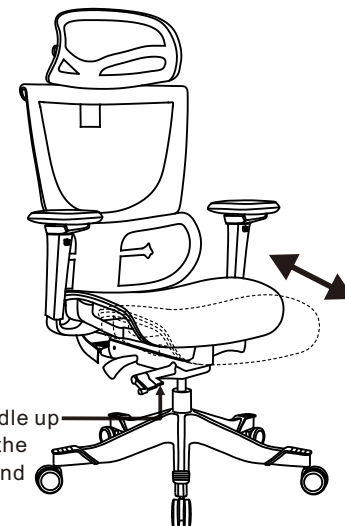


Lift the handle up and adjust the seat back and forth.


Step 7

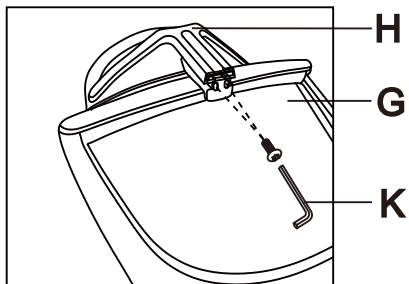


Step 8

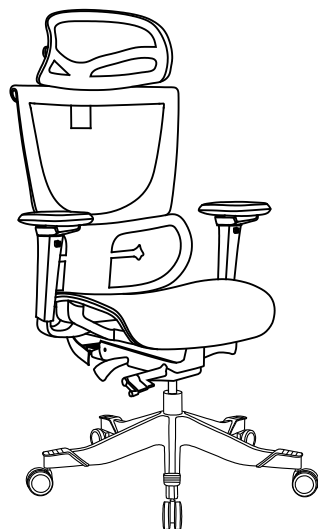

Function 2

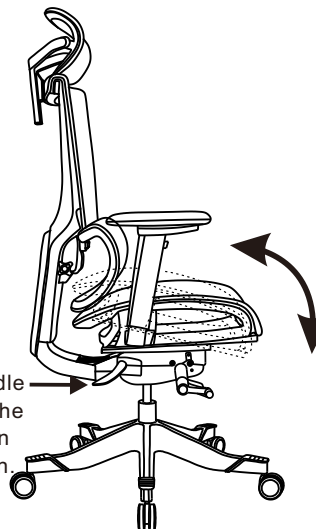

Lift the handle and adjust the seat cushion up and down.

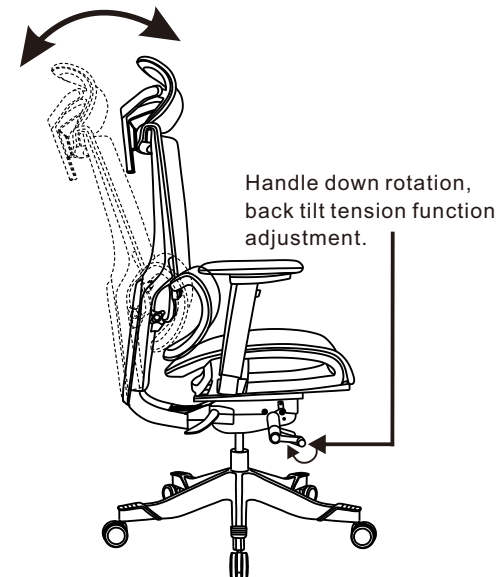

Handle down rotation, back tilt tension function adjustment.